






Characteristics

Orange - The universal symbol for Caution - and ideal for EMS, police and fire, haz mat functions, spills, etc. This medium weight nitrile glove is extremely elastic and comfortable while providing the tensile strength required for these demanding procedures. Polymer interior for rapid donning. Textured finish for an excellent grip even in the presence of moisture. Color: CAUTION Orange.

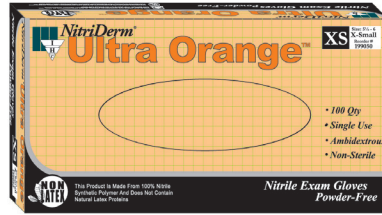

**Exam Glove
Non-Sterile**

**NitriDerm®
Ultra Orange™
Nitrile
Series 199**

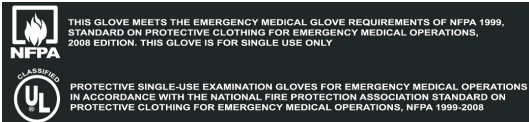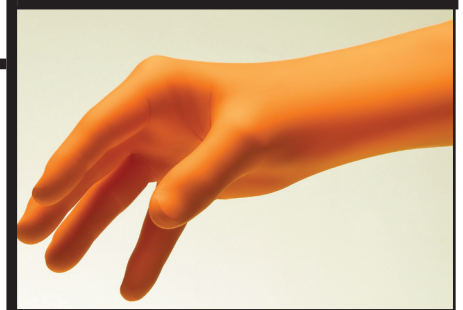

PRODUCT DETAILS

SIZE	ITEM NO.	PACKAGING	DESCRIPTION
XS	199050	100 Gloves/box, 10 boxes/case	Gloves, Exam, Nitrile, Non-Sterile, Powder-Free, Textured
S	199100	100 Gloves/box, 10 boxes/case	
M	199200	100 Gloves/box, 10 boxes/case	
L	199300	100 Gloves/box, 10 boxes/case	
XL	199350	100 Gloves/box, 10 boxes/case	
XXL	199400	90 Gloves/box, 10 boxes/case	

Features

- **NFPA & UL Certified**
- **Low Modulus**
- **Non-Latex**
- **Textured Finish**
- **Caution Orange Color**

Benefits

- **Quality Assurance**
- **Softer, More Comfortable Fit**
- **No Risk of Latex Allergens**
- **Improved Wet/Dry Grip**
- **More Easily Seen at Night**

Product Solutions You Trust




**INNOVATIVE
HEALTHCARE
CORPORATION**

www.ihcsolutions.com

Specification Sheet

NitriDerm[®] Ultra Orange[™]

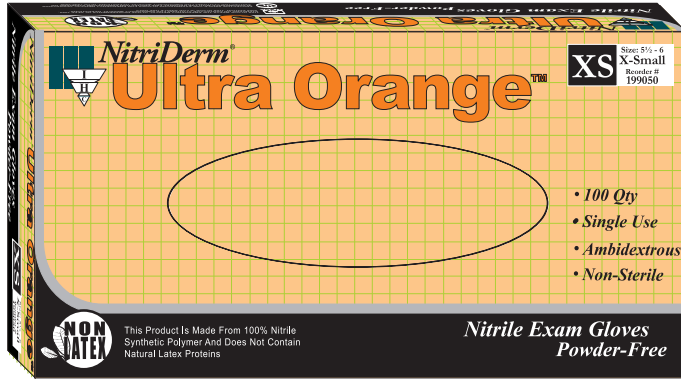

**Nitrile Exam Gloves
Powder-Free**



THIS GLOVE MEETS THE EMERGENCY MEDICAL GLOVE REQUIREMENTS OF NFPA 1999, STANDARD ON PROTECTIVE CLOTHING FOR EMERGENCY MEDICAL OPERATIONS, 2008 EDITION. THIS GLOVE IS FOR SINGLE USE ONLY



PROTECTIVE SINGLE-USE EXAMINATION GLOVES FOR EMERGENCY MEDICAL OPERATIONS IN ACCORDANCE WITH THE NATIONAL FIRE PROTECTION ASSOCIATION STANDARD ON PROTECTIVE CLOTHING FOR EMERGENCY MEDICAL OPERATIONS, NFPA 1999-2008

NitriDerm Ultra Orange is manufactured in compliance with the following international standards

Designation	Standard
ASTM D6319-00a(2005)	Standard Specification for Nitrile Examination Gloves for Medical Application
ASTM D5151-06	Standard Test Method for Detection of Holes in Medical Gloves
ASTM F1671-03	Standard Test Method for Resistance of Materials Used in Protective Clothing to Penetration by Blood-Borne Pathogens

Sizes XS-XL
100 Gloves/Box, 10 Boxes/Case

Sizes XXL
90 Gloves/Box, 10 Boxes/Case

Size	Item Number	Palm Width +/- 3mm	Total Length +/- 5mm	Thickness Finger mil	Thickness Finger mm
X-SMALL	199050	76	240	4	0.10
SMALL	199100	86	240	4	0.10
MEDIUM	199200	98	240	4	0.10
LARGE	199300	107	240	4	0.10
X-LARGE	199350	115	240	4	0.10
XX-LARGE	199400	125	240	4	0.10

Tensile Strength & Elongation	Before Aging	After Accelerated Aging
Tensile Strength Min. (Mpa)	14	14
ASTM Requirement Min. (Mpa)	14	14
Elongation Minimum Min. (%)	500	400
ASTM Requirement Min. (%)	500	400

**INNOVATIVE
HEALTHCARE
CORPORATION**

Product Solutions You Trust

1-800-272-1533



Innovative Healthcare Corporation is certified to both ISO 9001:2008 quality management system and ISO 13485:2003 quality management system for medical devices.